

# Configuration Sheet – Shorts


Commission no./ Patient ID:  
(No Name!)

## Step 1: What is ordered?

- |  |                                 |                              |  |
|--|---------------------------------|------------------------------|--|
| <input type="radio"/> <b>evomove orthokit</b> (incl. holder)         | <input type="radio"/> right leg | <input type="radio"/> female | Fabric color<br>● <input type="radio"/> grey ● <input type="radio"/> black |
| <input type="radio"/> <b>evomove solokit</b> (incl. pocket)          | <input type="radio"/> left leg  | <input type="radio"/> male   |  |
| <input type="radio"/> <b>Pair of new shorts</b> (excl. control unit) |                                 |                              |  |
| Reference (Ordernumber, patient ID,..): _____                        |                                 |                              |  |


## Step 2: Measurement (mandatory!)

### Circumferences

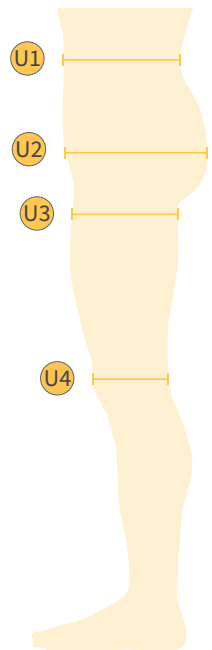


|  |             |              |
|--|-------------|--------------|
| <b>U1</b><br>Waist<br>(midway between the lower costal arch and the iliac crest, level with the navel) | cm          |              |
| <b>U2</b><br>Buttocks<br>(strongest part buttocks/hips)  | cm          |              |
| <b>Important:</b><br>Please measure both legs.   | <b>left</b> | <b>right</b> |
| <b>U3</b><br>Thigh<br>(1cm below crotch)   | cm          | cm           |
| <b>U4</b><br>Knee circumference<br>(back of the knee)  | cm          | cm           |

### Lengths

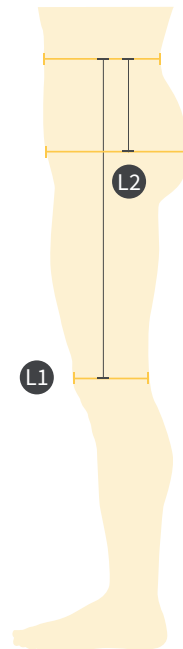

Body dimensions are measured, e.g. using a **rubber band to mark** the positions **U1, U2** and **U4**.

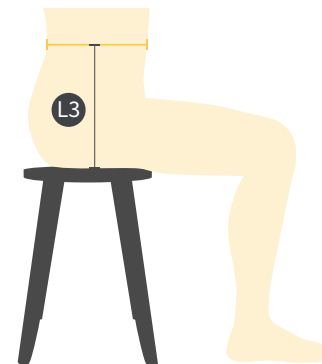


|  |    |
|--|----|
| <b>L1</b><br>Knee length<br>(Waist to knee circumference U4)       | cm |
| <b>L2</b><br>Buttocks<br>(Waist – strongest point on the buttocks) | cm |
| <b>L3</b><br>Seat length<br>(Waist to seat)                        | cm |
| <b>Body height</b>   | cm |

**Important:** The seat should be straight and without padding.

### Step 3: Detection of the electrode position (please check)

○

#### 1. Option: 3D-Scan

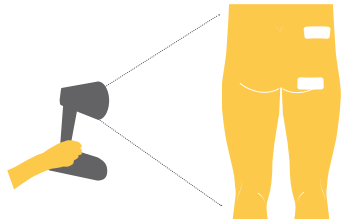


Create a **3D scan** using a scanner.

We accept **.obj** and **.stl** files.

**Important:** When scanning, please make sure that the buttocks and both legs can be seen standing from knee to waist.

○

#### 2. Option: Photos

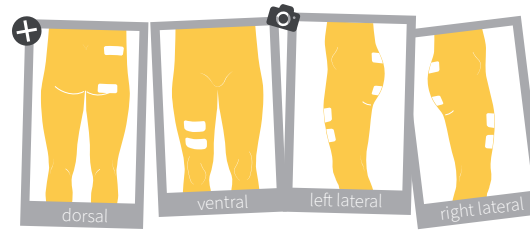

**Photo** with corresponding electrodes.

**Important:** Both legs must be visible from waist to knee when photographed.

**Do not forget:** Photograph laterally from both sides.

### Step 4: Details of the shorts

1

Cord in waistband

No  
 Yes



2

Handypocket

none  
 2a right  
 2b left

3

Pocket for evomove® control unit

3a right |  medial |  lateral  
 3b left |  medial |  lateral



4

Zipper  
(Desired position may be adjusted depending on the electrode position)

No  
 Yes, in the waistband  
 4a right |  short |  long  
 4b center |  short |  long  
 4c left |  short |  long

Yes, on the leg  
 4d right |  short |  long  
 4e left |  short |  long

Cable outlet  
(standard in the pocket of the evomove® control unit)

individual  
(please highlight in the picture)

Wearing height

Waist shorts |  Hipster shorts